



(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2020/0406260 A1**

Beebe et al. (43) **Pub. Date: Dec. 31, 2020**

(54) **VOLUME-FREE REAGENT ADDITION AND EXCLUSION-BASED SAMPLE PREPARATION FOR STREAMLINED MULTI-STEP ASSAYS**

(52) **U.S. Cl.**
CPC ... **B01L 3/502746** (2013.01); **B01L 3/502784** (2013.01); **B01L 3/502715** (2013.01); **G01N 33/54326** (2013.01); **B01L 2400/043** (2013.01); **B01L 2200/0673** (2013.01); **B01L 2200/16** (2013.01); **B01L 2300/0864** (2013.01); **B01L 2200/0642** (2013.01)

(71) Applicant: **Wisconsin Alumni Research Foundation**, Madison, WI (US)

(72) Inventors: **David J. Beebe**, Monona, WI (US); **Joshua M. Lang**, Madison, WI (US); **Duane S. Juang**, Madison, WI (US); **Scott M. Berry**, Madison, WI (US); **Tamara S. Rodems**, Madison, WI (US)

(57) **ABSTRACT**

A method of sample preparation for streamlined multi-step assays is provided. The method includes the step of providing a microfluidic device including a reservoir defined by a surface configured to repel an aqueous solution. A dried reagent is provided on a portion of the surface and the reservoir is filled with an oil. A first droplet formed from the aqueous solution is positioned on the dried reagent so to pick-up and re-dissolve the dried reagent therein so as to expose the portion of the surface. In addition, a second droplet of an aqueous solution may be deposited on a hydrophilic spot patterned on the surface. A magnetic force may be configured to interact magnetically with the paramagnetic beads within the first droplet to move the droplet through the oil in the reservoir or to move the paramagnetic beads from the first droplet, through the oil, into the second droplet.

(21) Appl. No.: **16/912,986**


(22) Filed: **Jun. 26, 2020**

Related U.S. Application Data

(60) Provisional application No. 62/868,296, filed on Jun. 28, 2019.

Publication Classification

(51) **Int. Cl.**
B01L 3/00 (2006.01)
G01N 33/543 (2006.01)

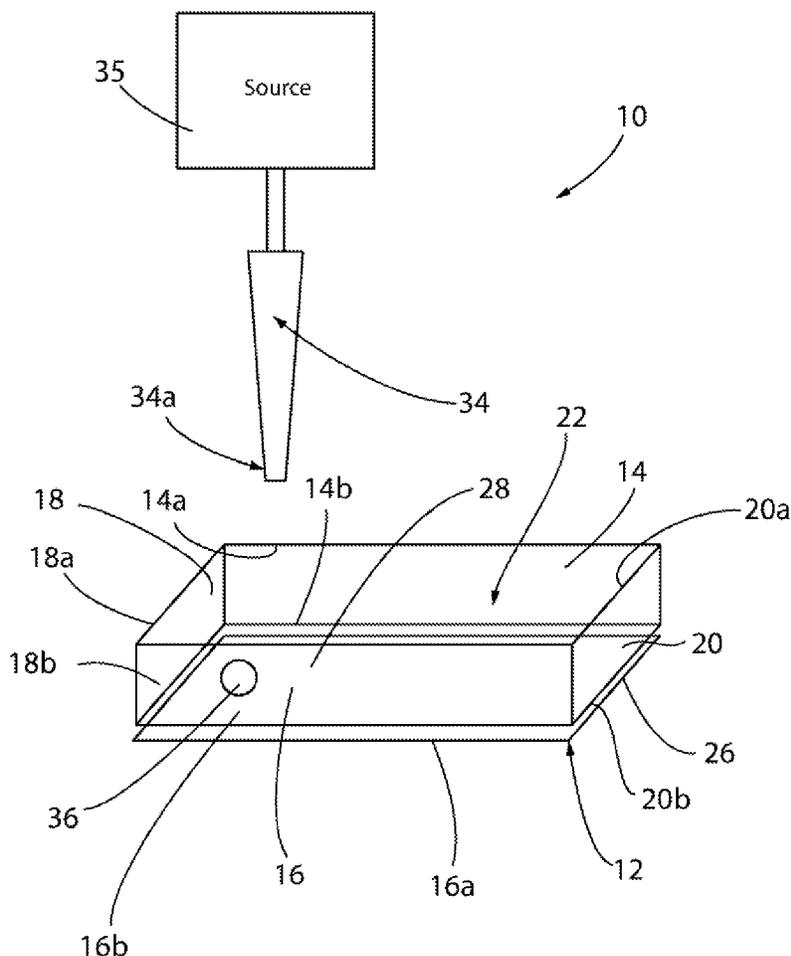

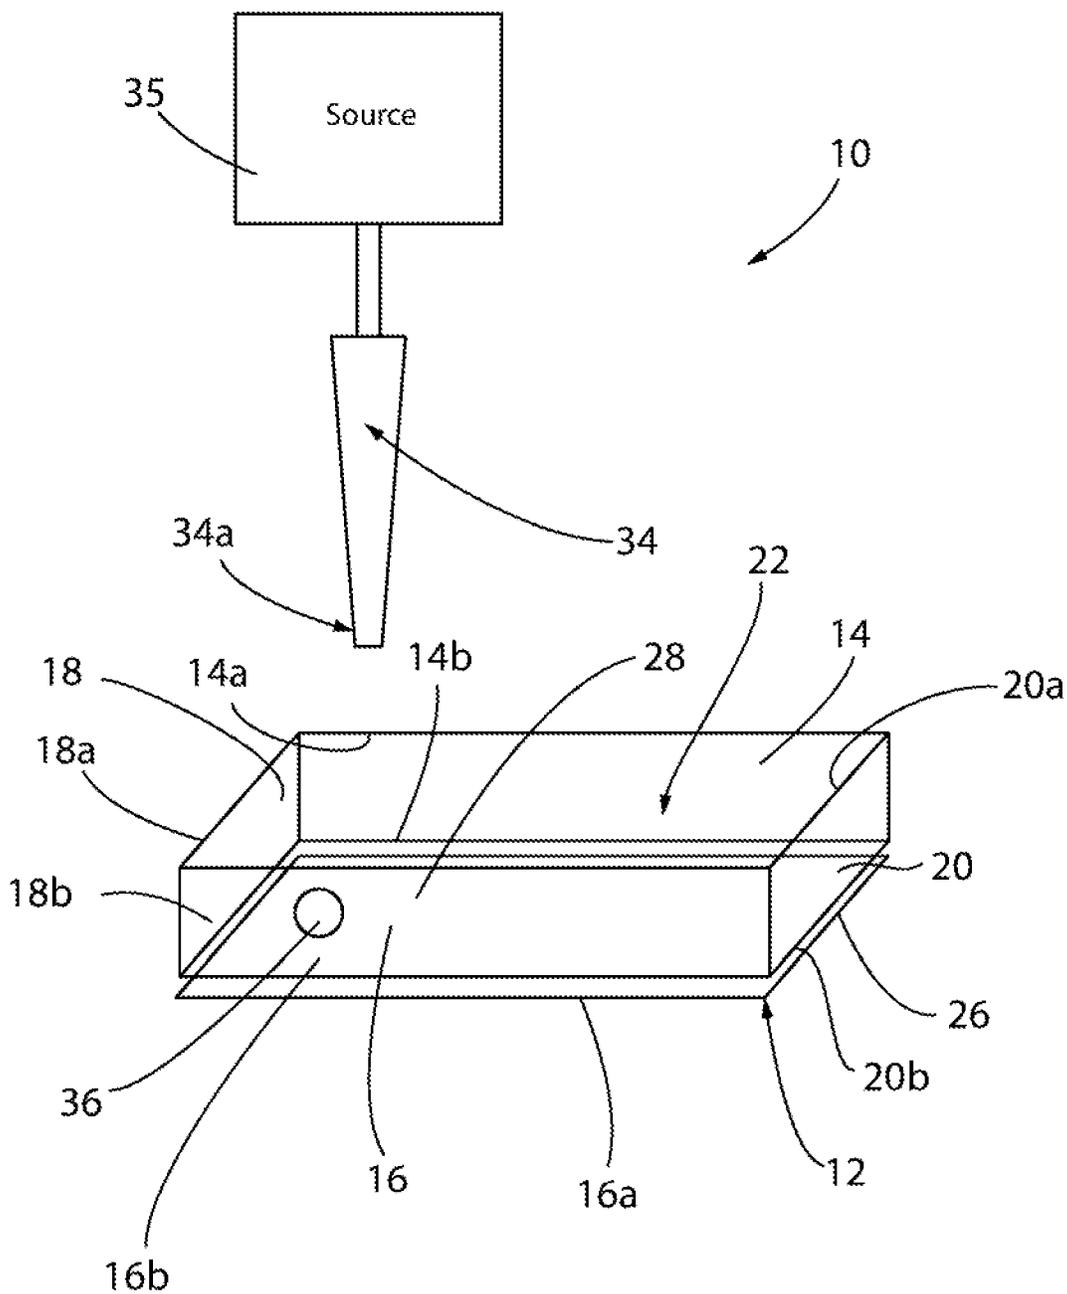
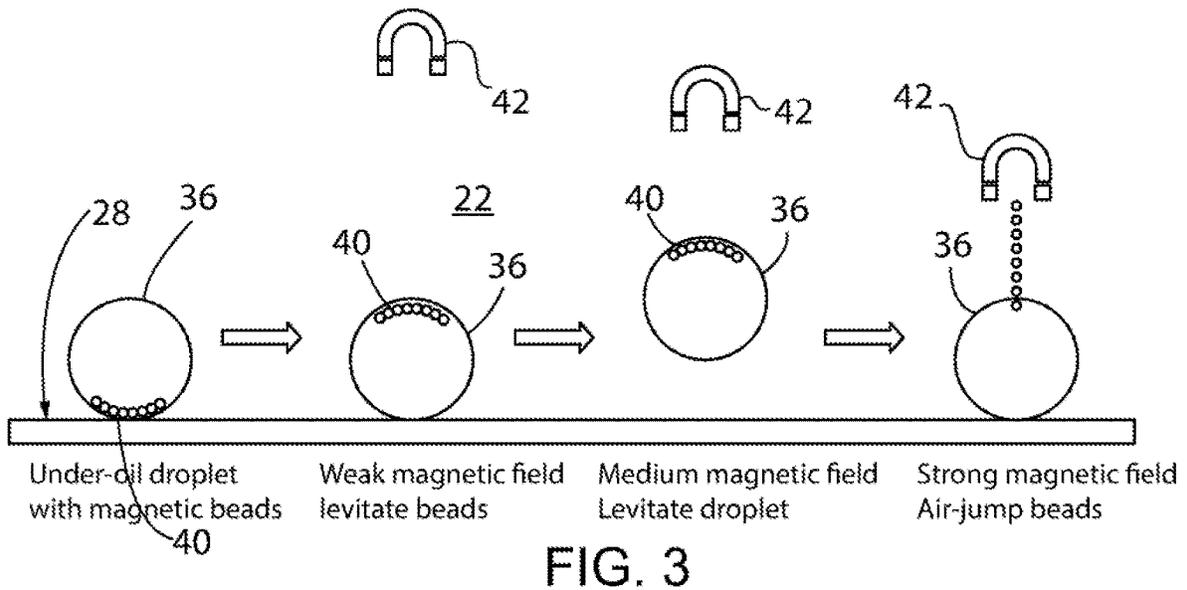
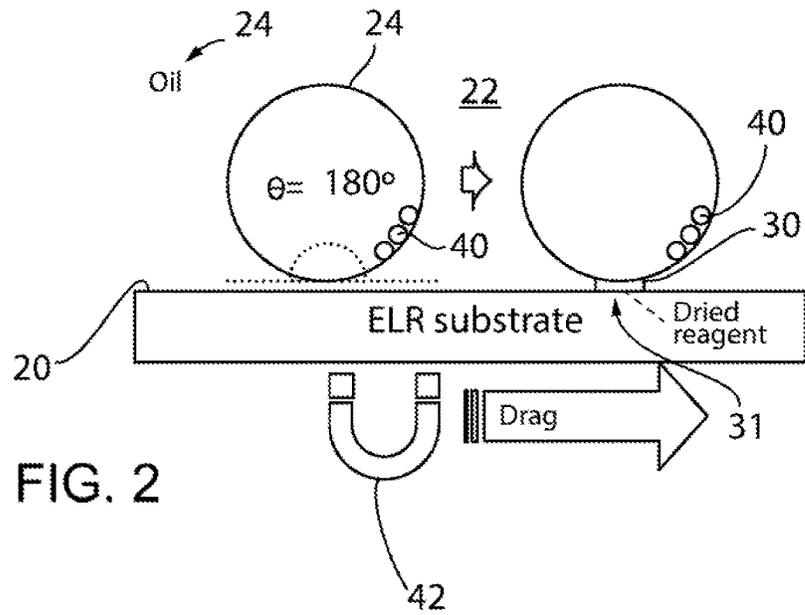


FIG. 1



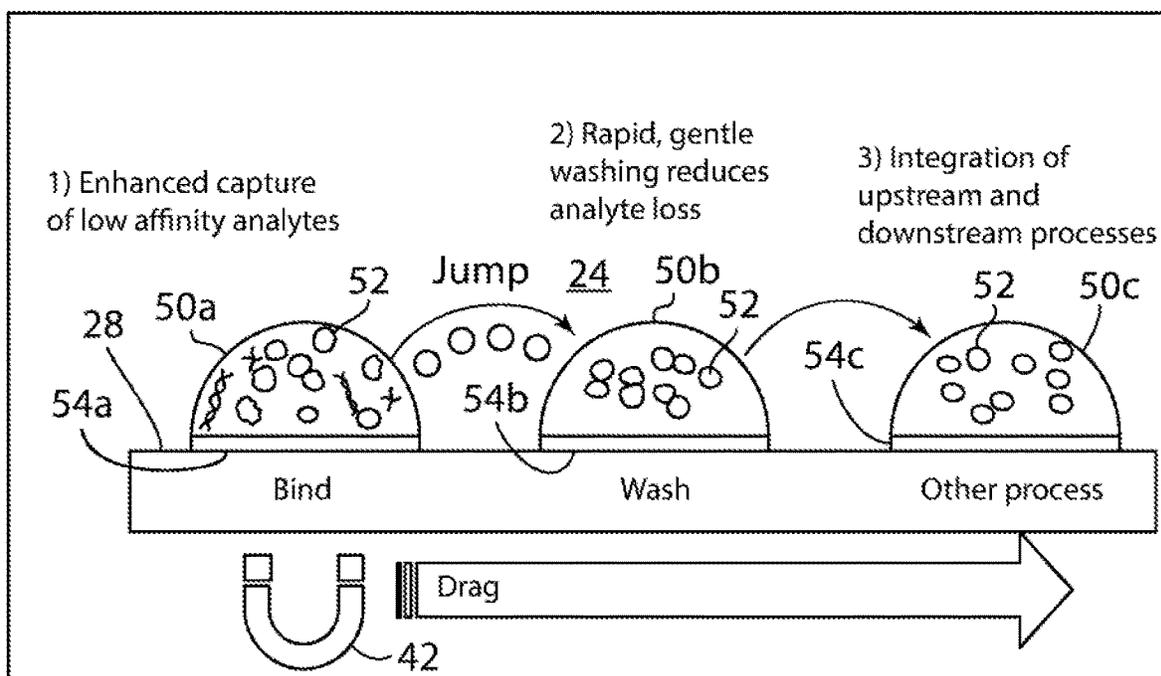


FIG. 4

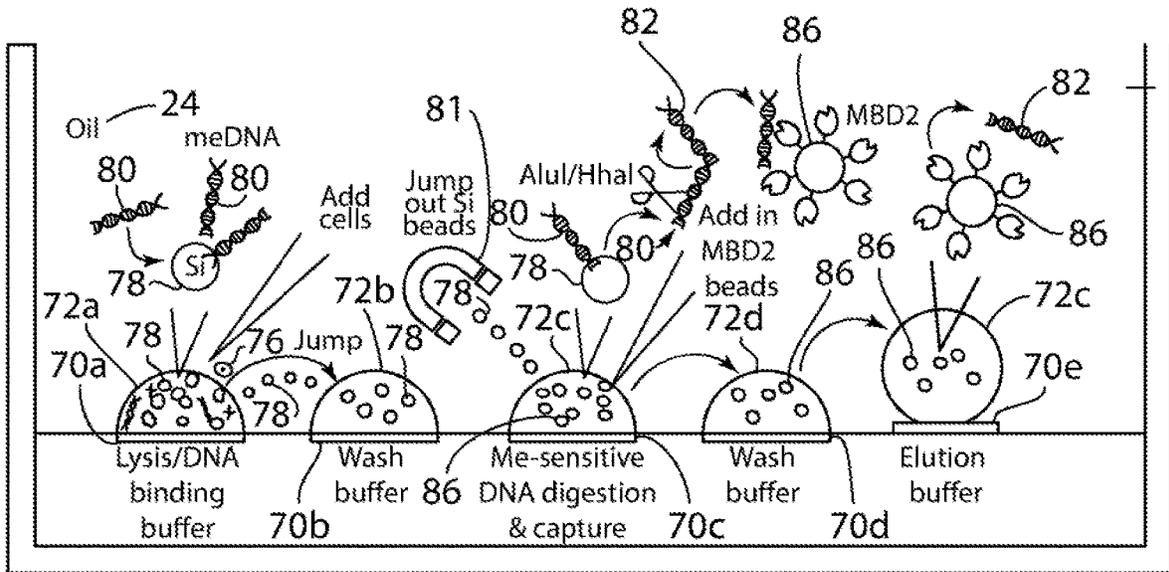


FIG. 5

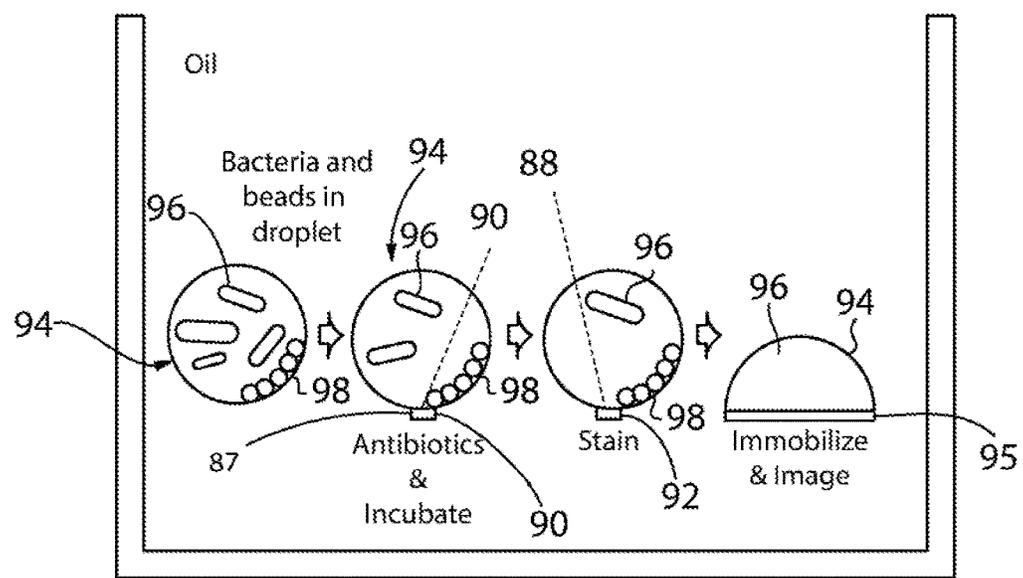


FIG. 6

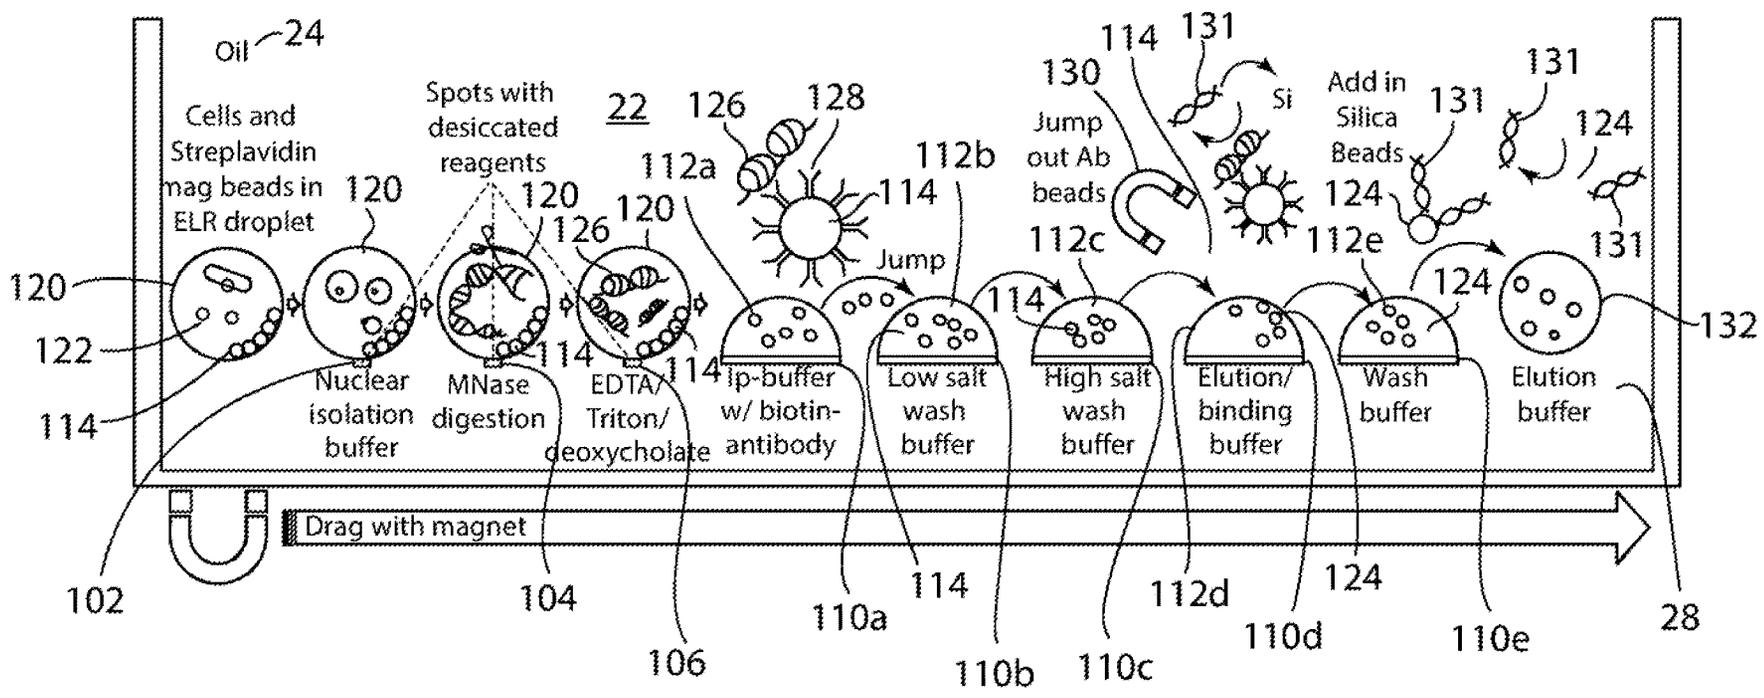


FIG. 7

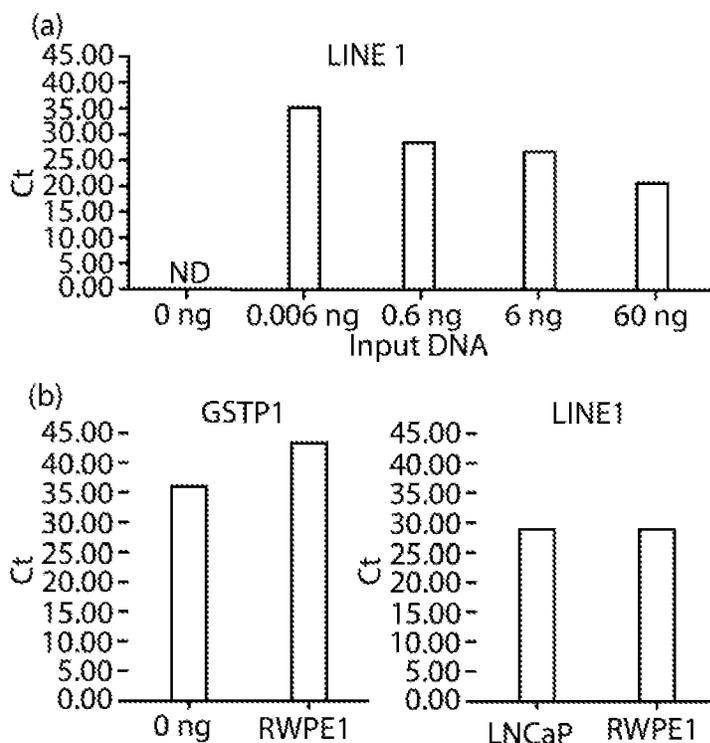


FIG. 8

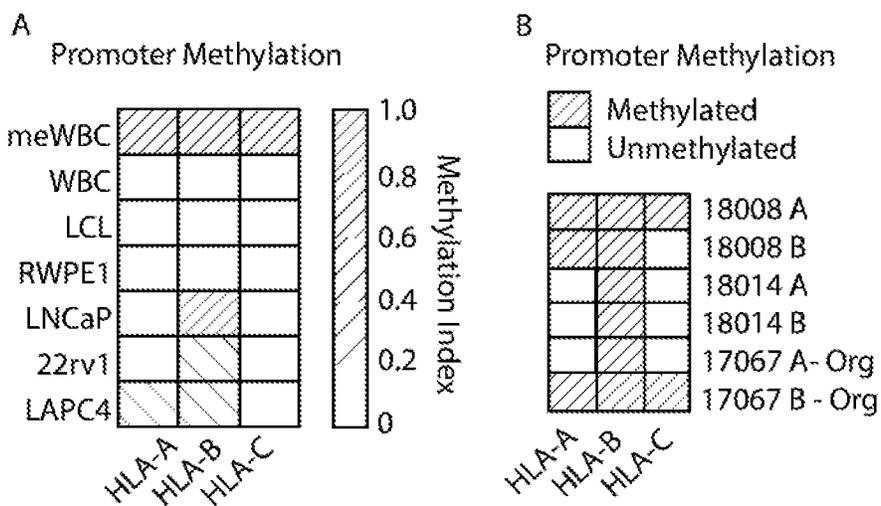


FIG. 9

**VOLUME-FREE REAGENT ADDITION AND
EXCLUSION-BASED SAMPLE
PREPARATION FOR STREAMLINED
MULTI-STEP ASSAYS**

**CROSS-REFERENCE TO RELATED
APPLICATION**

[0001] This application claims benefit from U.S. Provisional Application Ser. No. 62/868,296, filed Jun. 28, 2019, the entirety of which is incorporated herein.

REFERENCE TO GOVERNMENT GRANT

[0002] This invention was made with government support under CA81648 awarded by the National Institutes of Health and W81XWH-16-1-0514 awarded by the ARMY/ARO. The government has certain rights in the invention.

FIELD OF THE INVENTION

[0003] This invention related generally to microfluidics, and in particular, to a system and method for volume-free reagent addition and exclusion-based sample preparation for streamlined multi-step assays.

**BACKGROUND AND SUMMARY OF THE
INVENTION**

[0004] Liquid handling in nearly all assays can be primarily divided into two main categories: 1) adding a reagent into a pre-existing liquid phase (such as adding drugs to cell culture media) in which the target analyte (such as cells) can either be immobilized to a solid surface (adherent cells on the bottom of a dish) or reside in the liquid phase (such as non-adherent cells suspended in media); and 2) solution exchange, in which the target analyte has to be immobilized to a solid surface (such as cells attached to the bottom of a dish or antibodies immobilized to the bottom of an ELISA plate) and the liquid phase is mostly removed and replaced with another liquid phase (for changing solution conditions or washing). Although these operations can usually be performed reliably and with ease using a pipette in traditional macro-scale assays, it becomes much harder, and in many cases impossible, to perform for microscale assays with very small liquid volumes. Further, these operations often yield unreliable and problematic results. For example, in a macroscale assay, addition of 1 microliter (μL) of reagent to 1000 μL of solution only increases the total volume of the solution by approx. 0.1% which usually has little effect in terms of dilution of the original solution. However, adding the same 1 μL of reagent to a 1 μL microscale droplet would double the total volume of the droplet. Hence, any molecules already present in the original solution would be diluted by 50%.

[0005] Similarly, when performing a solution exchange, the residual liquid remaining on the solid surface after aspiration accounts for a very small percentage of the total assay volume and is often negligible. However, it becomes a much more significant problem in microscale assays due to the much higher surface to volume ratio. Thus, new strategies that can be utilized to perform reagent addition or a solution exchange without significantly perturbing the final volume of the assay would greatly benefit the field of microscale assays as a whole.

[0006] In view of the foregoing, it is a primary object and feature of the present invention to provide a method of a

method of sample preparation for streamlined multi-step assays that allows for the volume-free addition of a reagent to a sample.

[0007] It is a further object and feature of the present invention to provide a method of sample preparation for streamlined multi-step assays that allows for the preparation of an exclusion-based sample during a solution exchange.

[0008] It is a still further object and feature of the present invention to provide a method of sample preparation for streamlined multi-step assays that is simple and inexpensive to practice.

[0009] In accordance with the present invention, a method of sample preparation for streamlined multi-step assays is provided. The method includes the step of providing a microfluidic device including a reservoir defined by a surface configured to repel an aqueous solution. A dried reagent is provided on a portion of the surface. The reservoir is filled with an oil and a droplet of the aqueous solution is positioned on the dried reagent. The droplet picks-up and re-dissolves the dried reagent therein so as to expose the portion of the surface.

[0010] The step of providing the dried reagent on the portion of the surface includes the additional steps depositing the reagent on the surface and allowing reagent to dry and physically adsorb onto surface. The droplet may include paramagnetic beads therein. The step of positioning the droplet of the aqueous solution on the dried reagent may include the steps of generating a magnetic force and positioning the magnetic force to interact magnetically with the paramagnetic beads within the droplet. The magnetic force is moved to initiate corresponding movement of the droplet to the portion of the surface.

[0011] A hydrophilic spot may be patterned on the surface at a second location. The droplet with the dissolved reagent therein may be moved to the hydrophilic spot and pinned at the hydrophilic spot. The step of moving the droplet with the dissolved reagent to the hydrophilic spot may include the additional steps of positioning the magnetic force to interact magnetically with the paramagnetic beads within the droplet and moving the magnetic force to initiate corresponding movement of the droplet to the hydrophilic spot.

[0012] The hydrophilic spot may be a first hydrophilic spot and the method may include the additional step of patterning a second hydrophilic spot on the surface at a third location. In addition, the aqueous solution may be a first aqueous solution and the droplet may be a first droplet. A second droplet of a second solution may be pinned at the second hydrophilic spot. The magnetic force may be positioned to interact magnetically with the paramagnetic beads within the first droplet. Movement of the magnetic force may be used to initiate corresponding movement of the paramagnetic beads from the first droplet to the second droplet.

[0013] The dried reagent may be a first dried reagent and the portion of the surface may be a first portion. A second dried reagent may be provided on a second portion of the surface. The second dried reagent on the second portion of the surface may be provided by depositing the second reagent on the second portion of the surface and allowing the second reagent to dry and physically adsorb onto the second portion of the surface. The magnetic force may interact magnetically with the paramagnetic beads within the droplet and moved to initiate corresponding movement of the droplet to the second portion of the surface. The second dried

reagent may be picked-up and re-dissolved in the droplet so as to expose the second portion of the surface.

[0014] In accordance with a further aspect of the present invention, a method of sample preparation for streamlined multi-step assays is provided. The method includes the step of providing a microfluidic device including a reservoir defined by a surface configured to repel aqueous solutions. First and second hydrophilic spots are patterned at corresponding first and second locations of the surface. The reservoir is filled with an oil. A first droplet of a first aqueous solution is deposited on the first hydrophilic spot and a second droplet of a second aqueous solution is deposited on the second hydrophilic spot. The first droplet includes paramagnetic beads. The first droplet may be pinned at the first hydrophilic spot and the second droplet may be pinned at the second hydrophilic spot. A magnetic force is generated and configured to interact magnetically with the paramagnetic beads within the first droplet. The magnetic force is moved to initiate corresponding movement of the paramagnetic beads from the first droplet, through the oil, into the second droplet.

[0015] A dried reagent may be provided at a third location the surface prior to filling the reservoir with oil. The step of providing the dried reagent on the portion of the surface may include the additional steps depositing the reagent in a third aqueous solution on the surface and allowing the third aqueous solution to dry such that a dried reagent is physically adsorbed onto surface. A third droplet of a third aqueous solution may be positioned on the dried reagent. The third droplet picking-up and re-dissolving the dried reagent therein so as to expose the portion of the surface. The paramagnetic beads may be initially in the third droplet and the method may include the additional steps of positioning the magnetic force to interact magnetically with the paramagnetic beads within the third droplet and moving the magnetic force to initiate corresponding movement of the paramagnetic beads from the third droplet, through the oil, into the first droplet. Alternatively, the magnetic force may be moved to initiate corresponding movement of the third droplet into fluid communication with the first droplet. It is further contemplated with the paramagnetic bead with the second droplet to position the magnetic force to interact magnetically with the paramagnetic beads within the second droplet and move the magnetic force to initiate corresponding movement of the paramagnetic beads from the second droplet, through the oil, into the third droplet. Thereafter, the magnetic force may interact magnetically with the paramagnetic beads within the third droplet and initiate movement of the paramagnetic beads from the third droplet.

BRIEF DESCRIPTION OF THE DRAWINGS

[0016] The drawings furnished herewith illustrate a preferred methodology of the present invention in which the above advantages and features are clearly disclosed as well as others which will be readily understood from the following description of the illustrated embodiment.

[0017] In the drawings:

[0018] FIG. 1 is a schematic view of a system for effectuating the methodologies for volume-free reagent addition and exclusion-based sample preparation for streamlined multi-step assays;

[0019] FIG. 2 is a schematic, side elevational view of the system of FIG. 1 depicting a first arrangement thereof wherein the system is used in the volume-free addition of a reagent to a sample;

[0020] FIG. 3 is a schematic, side elevational view of the system of FIG. 1 depicting contact-free manipulation of a droplet having paramagnetic beads therein;

[0021] FIG. 4 is a schematic, side elevational view of the system of FIG. 1 depicting a second arrangement thereof wherein the system is used to perform exclusion-based sample preparation;

[0022] FIG. 5 is a schematic, side elevational view of the system of FIG. 1 depicting a third arrangement thereof wherein the system is used for the extraction of methylated-DNA (meDNA) from rare samples;

[0023] FIG. 6 is a schematic, side elevational view of the system of FIG. 1 depicting a fourth arrangement thereof wherein the system is used for antimicrobial susceptibility testing;

[0024] FIG. 7 is a schematic, side elevational view of the system of FIG. 1 depicting a fifth arrangement thereof wherein the system is used for extraction of chromatin-bound DNA from cells or tissues;

[0025] FIG. 8 are graphical charts showing (a) Ct values of extracted LINE1 meDNA from LNCaP cells with varying amounts of input DNA; and (b) Ct values of GSTP1 and LINE1 extracted methylated DNA from LNCaP prostate cancer and RWPE1 normal prostate cell lines using 0.6 ng input DNA; and

[0026] FIG. 9 are graphical charts showing (A) methylation status within the promoters of HLA-A, HLA-B, and HLA-C determined in cell lines and white blood cell (WBC) DNA wherein the methylation index is the ratio of methylated DNA in the enriched sample to methylated DNA in the same amount of input enzymatically methylated WBC DNA (meWBC) and a methylation index of 1.0 indicates methylation at every gene copy; (B) methylation status within the promoters of HLA-A, HLA-B, and HLA-C determined in biopsies from primary prostate cancer wherein two tumor sites were sampled from each patient, indicated as A or B following patient number, and Org: organoid grown from tumor cells obtained from biopsy.

DETAILED DESCRIPTION OF THE DRAWINGS

[0027] Exclusive liquid repellency (ELR) is a phenomenon observed in solid-liquid-liquid three phase systems, where a solid surface shows complete repellency to a liquid (with a contact angle (CA)=180°) when exposed to a second liquid. This phenomenon is observed when a particular thermodynamic boundary condition is satisfied, for example, by the equation:

$$\gamma S/Lcp + \gamma Ldp/Lcp \leq \gamma S/Ldp \quad \text{Equation (1)}$$

wherein: γ is the interfacial tension; S is solid; Lcp is a liquid of continuous phase; and Ldp is a liquid of dispersed phase. As hereinafter described, ELR enables additional fluidic control in open aqueous fluid under oil provided for in the system of the present invention.

[0028] Referring to FIG. 1, a schematic drawing depicting a system for carrying out a first aspect of the methodology of the present invention is generally designated by the reference numeral 10. System 10 includes microfluidic device 12 defined by first and second generally parallel, spaced side walls 14 and 16 respectively, interconnected by

first and second generally parallel, spaced end walls **18** and **20**, respectively. First and second side walls **14** and **16** respectively, and first and second end walls **18** and **20**, respectively, define reservoir **22** for receiving a fluid, such as oil **24** or like, for reasons hereinafter described. Upper edges **14a** and **16a** of first and second side walls **14** and **16** respectively, and upper edges **18a** and **20a** of end walls **18** and **20**, respectively, define an opening **26** for allowing access to reservoir **22**. Lower edges **14b** and **16b** of first and second side walls **14** and **16** respectively, and lower edges **18b** and **20b** of end walls **18** and **20**, respectively, are interconnected by an exclusive liquid repellency (ELR) surface **28** which communicates with reservoir **22**. ELR surface **28** is a hydrophobic solid surface having specific surface chemical and physical conditions when in combination with a given oil phase **24** can repel aqueous solutions, as hereinafter described. It can be appreciated that while microfluidic device **10** has a generally rectangular, box-like configuration, other configurations are possible without deviating from the scope of the present invention.

[0029] It is contemplated for system **10** to be used in the volume-free addition of a reagent to a sample, FIG. 2. More specifically, with reservoir **22** dry and free of fluids, reagent **30** of interest in solution may be deposited onto ELR surface **28**. Reagent **30** is allowed to dry (such as by desiccation and/or lyophilization) and physically adsorb onto ELR surface **28**. It is contemplated to dry reagent **30** at a known location **31** or locations along ELR surface **28** in order to facilitate operation of microfluidic device **12** and/or integration of microfluidic device **12** with various liquid/fluid handling equipment. Once reagent **30** is dried on ELR surface **28**, reservoir **22** of microfluidic device **12** is filled with a selected fluid, such as oil **24**.

[0030] Injector **34**, FIG. 1, is operatively connected to a source **35** and is configured to deliver droplet **36** of an aqueous solution of interest in oil **24** in reservoir **22** of microfluidic device **12** at a desired location. It is intended for the aqueous solution from which droplet **36** is formed to be immiscible with oil **24** in reservoir **22**. Injector **34** may be configured to deliver droplet **36** of the aqueous solution directly into oil **24** (in other words, tip **34a** of injector **34** may be submerged within oil **24**). Alternatively, injector **34** may be configured to deliver droplet **36** by releasing droplet **36** above oil **24** and allowing gravity to bring droplet **36** into reservoir **22**. This arrangement is only suitable for conditions where droplet **36** is sufficiently dense relative to oil **24** and a person having ordinary skill in the art could determine the conditions under which this is achievable either by computational methods or by routine experimental optimization. In either instance described above with respect to the injector **34**, injector **34** may include a mechanism for urging droplet **36** out of tip **34a** of injector **34**. For example, such mechanism may include a plunger mechanism, a pump mechanism, such as a peristaltic pump, and the like. A computer (not shown) may be coupled to injector **34** and configured to control the introduction of droplet **36** into oil **24**.

[0031] It is contemplated for droplet **36** to include paramagnetic beads **40** and for system **10** to include magnetic manipulator **42** configured to interact magnetically with paramagnetic beads **40** within droplet **36** to initiate movement of the droplet **36** within oil **24**. Magnetic manipulator **42** can be handheld or can be coupled to an automated movement mechanism (not shown). The automated move-

ment mechanism may be operatively connected to a computer (not shown) configured to control magnetic properties of the magnetic manipulator **42** and/or to control the optional automated movement mechanism associated with magnetic manipulator **42**. By way of example, magnetic manipulator **42** may take the form of a magnet, an electromagnetic force generator, or the like.

[0032] Initially, magnetic manipulator **42** is utilized to draw droplet **36** over location **31** of the previously dried-up reagent **30** using magnetic manipulator **42**. With droplet **36** positioned over location **31** of the previously dried-up reagent **30**, droplet **36** picks-up and re-dissolves the desiccated reagent **30**, with virtually no increase in the total volume of droplet **36**. This phenomenon is possible due to the highly aqueous-repellent characteristic of ELR surface **28** under oil **24**, which allows near complete recovery of the dried-up reagent by the aqueous droplet **36**.

[0033] It can be understood that prior to depositing oil **24** in reservoir **22**, a plurality of different reagents of interest in solution may be deposited onto ELR surface **28** and be allowed to dry and physically adsorb onto ELR surface **28** at known, corresponding locations. With the plurality of reagents dried on ELR surface **28**, droplet **36** may be sequentially drawn to each of the known locations by magnetic manipulator **42**, e.g. manually or by means of an automated movement mechanism, thereby enabling the multi-step addition of the plurality of different reagents via the sequentially dragging of droplet **36** along ELR surface **28** without adding to the total volume of droplet **36**. It is contemplated to provide indicia along or adjacent to ELR surface **28** to allow an individual or the automated movement mechanism to accurately identify the known locations of the plurality of reagents dried on ELR surface **28**.

[0034] Referring to FIG. 3, it is contemplated for paramagnetic beads **40** within droplet **36** to be employed to enhance and mix the plurality of reagents within droplet **36** by moving magnetic manipulator **42** a desired pattern, for example, by moving magnetic manipulator **42** up and down. It is further contemplated by manipulating the distance between magnetic manipulator **42** and paramagnetic beads **40**, various droplet/bead manipulations can be performed, including sideways movement of droplet **36** within reservoir **22**, the internal mixing of droplet **36**, and the levitation of droplet **36** within reservoir **22**. In addition, by increasing the magnetic force on paramagnetic beads **40** in droplet **36**, for example, by moving magnetic manipulator **42** closer to droplet **36**, paramagnetic beads **40** “jump” out of droplet **36** entirely. This, in turn, enables the recovery of analytes bound to paramagnetic beads **40**. With paramagnetic beads **40** removed from droplet **36**, droplet **36** is rendered inactive from further magnetic manipulation.

[0035] System **10** may also be used for effectuating a methodology for exclusion-based sample preparation (ESP), FIG. 4. More specifically, it is contemplated to utilize system **10** to perform sequential liquid exchanges by dragging functionalized paramagnetic beads **52** using a magnetic force generated by magnetic manipulator **42** from an aqueous phase through an immiscible oil barrier to fully “exclude” non-target analytes and into another aqueous phase to perform a rapid and single-step liquid exchange.

[0036] An array of hydrophilic spots **54a-54c** are pre-patterned on ELR surface **28** of microfluidic device **12**. As heretofore described, ELR surface **28** is a hydrophobic solid surface having specific surface chemical and physical con-

ditions intended to repel aqueous solutions. One or more injectors **34** is configured to deliver a series of droplets **50a-50c** of selected compositions on corresponding hydrophilic spots **54a-54c**, respectively, on ELR surface **28**. For example, droplet **50a** may be composed of an aqueous solution having a desired analyte and functionalized paramagnetic beads **52** to which the desired analyte binds dispersed therein. Droplet **50b** may be composed of a buffer solution for washing away unbound analyte with the minimal loss of any analytes bound to the functionalized paramagnetic beads **52**. Droplet **50c** may be composed of a still further solution, such as an elution solution, to wash away any proteins unbound to functionalized paramagnetic beads **52**. It is also noted that a dried reagent (such as an immunoprecipitation (IP) buffer, an antibody, a low salt wash buffer, a high salt wash buffer, an elution buffer, a wash buffer, etc.), as heretofore described, may be provided on hydrophilic spots **54a-54c**. As such, a user need only deposit a droplet thereon to reconstitute the dried reagents. This arrangement allows microfluidic device **12** to be packaged as a single platform that includes all the necessary reagents to perform a desired assay. In either arrangement, it can be appreciated that the hydrophilic nature of the array of hydrophilic spots **54a-54c** on ELR surface **28** acts to pin droplets **50a-50c** thereon. In addition, the hydrophobic nature of ELR surface **28** further acts to retain droplets **50a-50c** on hydrophilic spots **54a-54c** of ELR surface **28**.

[0037] Once droplets **50a-50c** are deposited on corresponding hydrophilic spots **54a-54c**, respectively, on ELR surface **28**, magnetic manipulator **42** is positioned below ELR surface **28** such that a magnetic force generated by magnetic manipulator **42** magnetically attracts functionalized paramagnetic beads **52**. More specifically, magnetic manipulator **42** is positioned below hydrophilic spot **50a** of ELR surface **28** such that the magnetic force generated by magnetic manipulator **42** attracts the analyte-bound functionalized paramagnetic beads **52** in droplet **50a**. Thereafter, as magnetic manipulator **42** is slid axially along the underside of ELR surface **28** to a position below hydrophilic spot **50b** of ELR surface **28**, the magnetic force generated by magnetic manipulator **42** draws the analyte-bound functionalized paramagnetic beads **52** from droplet **50a**, through oil **24**, and into droplet **50b**. Due to the immiscible characteristics of oil **24** and aqueous phase of droplet **50a**, the aqueous liquid may be removed from analyte-bound functionalized paramagnetic beads **52**, thereby greatly reducing the residual liquid adsorbed on analyte-bound functionalized paramagnetic beads **52**. With analyte-bound functionalized paramagnetic beads **52** received in droplet **50b**, the buffer solution comprising droplet **50b** washes away any unbound analyte with the minimal loss of the analytes bound to analyte-bound functionalized paramagnetic beads **52**.

[0038] Once analyte-bound functionalized paramagnetic beads **52** is washed in droplet **50b**, magnetic manipulator **42** may be slid axially along the underside of ELR surface **28** from a position below hydrophilic spot **50b** of ELR surface **28** to a position below hydrophilic spot **50c** of ELR surface **28**, thereby drawing the analyte-bound functionalized paramagnetic beads **52** from droplet **50b**, through oil **24**, and into droplet **50c**. Again, due to the immiscible characteristics of oil **24** and aqueous phase of droplet **50b**, the aqueous liquid may be removed from analyte-bound functionalized paramagnetic beads **52**, thereby greatly reducing the residual liquid adsorbed on analyte-bound functionalized paramag-

netic beads **52**. With analyte-bound functionalized paramagnetic beads **52** received in droplet **50c**, the elution solution comprising droplet **50c** washes away any proteins unbound to analyte-bound functionalized paramagnetic beads **52**. Once analyte-bound functionalized paramagnetic beads **52** are washed in droplet **50c**, analyte-bound functionalized paramagnetic beads **52** may be removed from droplet **50c** by a magnetic force generated by magnetic manipulator **42** for further downstream processing. Alternatively, a magnetic force generated by magnetic manipulator **42** may be used to draw the analyte-bound functionalized paramagnetic beads **52** from droplet **50c**, through oil **24**, and into a downstream droplet (not shown) for further processing.

[0039] As described, the methodology for ESP heretofore described is inherently non-dilutive and more rapid than traditional techniques, thereby enabling higher analyte recovery and reduced sample loss. This, in turn, helps preserve molecular interactions between the desired analytes and the functionalized paramagnetic beads to which the desired analytes bind that are low affinity (high dissociation constant, K_d) or short lived (high interaction off-rate). Further, the functionalized paramagnetic beads may be moved from any given droplet to another in both the x and y directions, thereby allowing for more degrees of freedom of movement for the functionalized paramagnetic beads. It is further noted that the hydrophobic nature of ELR surface ensures that very little, if any, residual liquid is left behind on the functionalized paramagnetic beads as the functionalized paramagnetic beads are moved between droplets and prevents "invasion" or cross contamination between droplets when the functionalized paramagnetic beads are moved therebetween.

[0040] As hereinafter described, system **10** and the methodologies heretofore described may be used to effectuate various multi-step assays. By way of example, system **10** and the methodologies heretofore described may be used for: 1) methylated-DNA (meDNA) extraction from rare samples; 2) antimicrobial susceptibility testing; and 3) extraction of chromatin-bound DNA from cells or tissues.

[0041] Referring to FIG. 5, selective oxygen (**02**) plasma may be used to etch ELR surface **28** to create regions **70a-70e** of selective aqueous adhesion surrounded by ELR surface **28** that resist aqueous contact. Thereafter, reservoir **22** of microfluidic device **12** is filled with a selected fluid, such as oil **24**. After flooding the reservoir **22** with oil **24**, one of more injectors **34** are configured to deliver droplets **72a-72e** of desired aqueous solutions in oil **24** in reservoir **22** of microfluidic device **12** to corresponding regions **70a-70e**, respectively. It is intended for the aqueous solutions to be immiscible with oil **24** in reservoir **22**. More specifically, droplet **72a** may be composed of a lysis/DNA binding buffer; droplet **72b** may be composed of a wash buffer; droplet **72c** may be composed of a methylated-sensitive DNA digestion & capture solution; droplet **72d** may be composed of a wash buffer; and droplet **72e** may be composed elution buffer. As noted, the hydrophilic nature of regions **70a-70e** on ELR surface **28** acts to pin droplets **72a-72e** thereon. In addition, the hydrophobic nature of ELR surface **28** further acts to retain droplets **72a-72e** on regions **70a-70e** of ELR surface **28**.

[0042] Cells **76** are isolated into droplet **72a** and then lysed in situ by the lysis/DNA binding buffer thereby solubilizing DNA **80** of cells **76**. Functionalized paramagnetic beads **78** are added to droplet **72a** such that DNA **80** bind

thereto. Thereafter, magnetic manipulator 42 is positioned below region 70a of ELR surface 28 such that the magnetic force generated by magnetic manipulator 42 attracts the DNA-bound functionalized paramagnetic beads 78 in droplet 72a. Magnetic manipulator 42 is slid axially along the underside of ELR surface 28 to a position below region 70b of ELR surface 28 such that the magnetic force generated by magnetic manipulator 42 draws the DNA-bound functionalized paramagnetic beads 78 from droplet 70a, through oil 24, and into droplet 70b. Due to the immiscible characteristics of oil 24 and aqueous phase of droplet 70a, the aqueous liquid is removed from DNA-bound functionalized paramagnetic beads 78, thereby greatly reducing the residual liquid adsorbed on DNA-bound functionalized paramagnetic beads 78. With DNA-bound functionalized paramagnetic beads 78 received in droplet 70b, wash buffer solution of droplet 70b washes away any undesired material from DNA-bound functionalized paramagnetic beads 78 with the minimal loss of the DNA bound to DNA-bound functionalized paramagnetic beads 78.

[0043] Magnetic manipulator 42 is then slid axially along the underside of ELR surface 28 to a position below region 70c of ELR surface 28, the magnetic force generated by magnetic manipulator 42 draws DNA-bound functionalized paramagnetic beads 78 from droplet 70b, through oil 24, and into droplet 70c. Due to the immiscible characteristics of oil 24 and aqueous phase of droplet 70b, the aqueous liquid is removed from DNA-bound functionalized paramagnetic beads 78, thereby greatly reducing the residual liquid adsorbed on DNA-bound functionalized paramagnetic beads 78.

[0044] In order to ensure system 10 is sensitive enough to pull out meDNA against a large amount of background unmethylated DNA, two restriction enzymes, AluI and HhaI, are added to droplet 70c. AluI is intended to fragment DNA 80 bound to functionalized paramagnetic beads 78 and HhaI is intended to further digest DNA 80 only at unmethylated restriction recognition sites, thereby preserving meDNA fragments 82. Once DNA 80 bound to functionalized paramagnetic beads 78 is fragmented and digested at the unmethylated restriction recognized sites, functionalized paramagnetic beads 78 may be drawn from droplet 70c by means of a secondary magnetic source, such as magnet 81. Separately, paramagnetic beads are coupled with the methyl-CpG binding domain of methyl-CpG binding domain protein 2 (MBD2-MBD) via His-tag chemistry to form MBD2-MBD conjugated paramagnetic beads 86. As is known, methyl-DNA binding (MBD) proteins, such as MBD2 enable the isolation of meDNA after restriction enzyme-based digestion of total DNA. Paramagnetic beads 86 are introduced into droplet 70c and mixed with meDNA fragments 80 so to allow the MBD2-MBD protein coupled to paramagnetic beads 86 to bind to meDNA fragments 82 within droplet 70c.

[0045] With meDNA fragments 82 bound to functionalized paramagnetic beads 86 in droplet 70c, magnetic manipulator 42 is, once again, slid axially along the underside of ELR surface 28 to a position below region 70d of ELR surface 28 such that the magnetic force generated by magnetic manipulator 42 draws the functionalized paramagnetic beads 86 from droplet 70c, through oil 24, and into droplet 70d. Due to the immiscible characteristics of oil 24 and aqueous phase of droplet 70c, the aqueous liquid is removed from functionalized paramagnetic beads 86,

thereby greatly reducing the residual liquid adsorbed on functionalized paramagnetic beads 86. With functionalized paramagnetic beads 78 received in droplet 70d, wash buffer solution of droplet 70d washes away any undesired material from functionalized paramagnetic beads 86 with the minimal loss of meDNA fragments 82 bound to functionalized paramagnetic beads 86.

[0046] Once functionalized paramagnetic beads 86 are washed in droplet 70d, magnetic manipulator 42 is then slid axially along the underside of ELR surface 28 to a position below region 70e of ELR surface 28. The magnetic force generated by magnetic manipulator 42 draws functionalized paramagnetic beads 86 from droplet 70d, through oil 24, and into droplet 70e. Due to the immiscible characteristics of oil 24 and aqueous phase of droplet 70d, the aqueous liquid is removed from functionalized paramagnetic beads 86, thereby greatly reducing the residual liquid adsorbed on functionalized paramagnetic beads 86. Elution buffer of droplet 72e facilitates the elution of meDNA fragments 82 from functionalized paramagnetic beads 86. Functionalized paramagnetic beads 86 may be removed from droplet 72e by a magnetic force generated by a secondary magnetic force generator, e.g., a magnet (not shown), and transferred to a PCR tube (not shown), wherein functionalized paramagnetic beads 86 may be heated to a predetermined temperature (e.g., 95° C.) to cause elution of meDNA fragments 82 therefrom.

[0047] As described, by systematically arranging the sequence of the patterned hydrophilic spots on ELR surface 28, one can perform a streamlined reagent addition (lysis buffer), digestion (restriction enzymes), and extraction (capture by MBD2-modified paramagnetic beads) protocol by moving a magnet, without pipetting/liquid handling steps therebetween. The delivery of single cell lysis buffer into the droplets allows for the assay volume to remain low throughout the protocol to minimize analyte dilution and maximize recovery and binding.

[0048] To optimize the methodology of the present invention, it can be appreciated that routine alterations to the protocol as described above can be made. Such alterations may include: 1) Adjustments to the incubation times for cell lysis, the binding of the DNA and/or the DNA fragments to the functional paramagnetic beads, or restriction enzyme digestion to optimize the amount and purity of the output. Decreasing incubation times may reduce the amount of degradation of DNA or methylation signatures during the protocol. 2) Altering the magnetic bead chemistries for meDNA enrichment to increase meDNA recovery or purity. 3) Altering formulation of the elution buffers due to low sample yield.

[0049] With this method, detection of LINE1 meDNA from 0.006 ng of input human genomic DNA equivalent to approximately 1 cell is possible. Using LINE1 and GSTP1 methylation in cell lines as a model system, GSTP1 methylation in LNCaP prostate cancer cells may be detected, with little to no GSTP1 methylation signal from RWPE1 (which is normally non-methylated for GSTP1), FIG. 8. To test the ability to probe other epigenomic regions, meDNA enrichment was measured at HLA-A, HLA-B, and HLA-C in cancer cell lines where the RNA and protein expression is downregulated relative to noncancerous cell lines. As predicted, meDNA in cell lines with absent protein expression of HLA molecules (LAPC4, 22RV1 and LNCaP prostate cancer cell lines) was detected, but not in normal cells with

high expression of HLA (including white blood cells, RWPE1-normal prostate epithelial cells, and LCL lymphoid cells). To test the ability to detect meDNA in patient samples, meDNA enrichment was measured at HLA-A, HLA-B, and HLA-C in matched human prostate tumor biopsies, FIG. 9, meDNA was detected at each of these loci in some patient biopsies, with meHLA-B detection in 5/5 samples tested, thus confirming the feasibility and potential clinical relevance of the methodology of the present invention.

[0050] Referring to FIG. 6, it can be understood that system 10 may also be used to test for antimicrobial susceptibility. More specifically, with reservoir 22 dry and free of fluids, an antibiotic of interest 87 in solution may be deposited onto ELR surface 28 at a first location 90 and allowed to dry and physically adsorb onto ELR surface 28. In addition, a fluorescent bacteria stain 89 in solution may be deposited onto ELR surface 28 at a second location 92 and allowed to dry and physically adsorb onto ELR surface 28. Once the antibiotic of interest and the fluorescent bacteria stain are dried on ELR surface 28, reservoir 22 of microfluidic device 12 is filled with a selected fluid, such as oil 24.

[0051] In operation, injector 34 delivers droplet 94 of a desired volume, e.g., 2 μ L, containing bacteria 96 and paramagnetic beads 98 into reservoir 22. As heretofore described, magnetic manipulator 42 is configured to interact magnetically with paramagnetic beads 98 within droplet 94 to initiate movement of the droplet 94. As such, magnetic manipulator 42 may be utilized to draw droplet 94 over first location 90 of the previously dried antibiotic of interest. With droplet 94 positioned over location 90 of the previously dried antibiotic of interest, droplet 94 picks-up and re-dissolves the antibiotic of interest 87 over a desired incubation period, (e.g., 24 hours), with virtually no increase in the total volume of droplet 94. This phenomenon is possible due to the highly aqueous-repellent characteristic of ELR surface 28 under oil 24, which allows near complete recovery of the dried antibiotic of interest by the aqueous droplet.

[0052] After the incubation period, magnetic manipulator 42 is utilized to drag droplet 94 through oil 24 to second location 92, wherein the fluorescent bacteria stain was previously dried. With droplet 94 positioned over second location 92 of the previously dried fluorescent bacteria stain 89, droplet 94 picks-up and re-dissolves the fluorescent bacteria stain for a desired time period, with virtually no increase in the total volume of droplet 94. As is known, any viable bacterial cells in droplet 94 after exposure to the antibiotic of interest will be stained by fluorescent bacteria stain 89 and may be detected by fluorescent microscopy. Once the viable bacterial cells in droplet 94 are stained by the fluorescent bacteria stain, magnetic manipulator 42 may be utilized to drag droplet 94 through oil 24 to hydrophilic spot 95 to pre-patterned on ELR surface 28 so as to immobilize droplet 94 thereon. Thereafter, fluorescent imaging of droplet 94 may be performed so as to allow for detection of any viable bacterial cells therein.

[0053] Referring to FIG. 8, it is further contemplated to utilize system 10 to extract chromatin-bound DNA from cells or tissues. More specifically, with reservoir 22 dry and free of fluids, a nuclear isolation buffer is deposited onto ELR surface 28 at a first location 102 and allowed to dry and physically adsorb onto ELR surface 28. In addition, a micrococcal nuclease (MNase) digestion solution is depos-

ited onto ELR surface 28 at a second location 104 and allowed to dry and physically adsorb onto ELR surface 28. A buffer such as a ethylenediaminetetraacetic acid (EDTA)/Triton/deoxycholate solution is deposited onto ELR surface 28 at a third location 106 and allowed to dry and physically adsorb onto ELR surface 28.

[0054] In addition, an array of hydrophilic spots 110a-110e are pre-patterned on ELR surface 28 of microfluidic device 12. It is intended for one or more injectors 34 to be configured to deliver a series of droplets 112a-112e of selected compositions on corresponding hydrophilic spots 110a-110e, respectively, on ELR surface 28. For example, droplet 110a may be composed of immunoprecipitation (IP) buffer containing biotinylated antibodies for facilitating the antibody-mediated capture of chromatin. Droplet 112b may be composed of a low salt wash buffer solution for washing away unbound reagents with the minimal loss of any chromatin bound to streptavidin paramagnetic beads 114, as hereinafter described. Droplet 112c may be composed of a high salt wash buffer solution for washing away unbound reagents with the minimal loss of any chromatin bound to the streptavidin paramagnetic beads 114. Droplet 112d may be composed of an elution/binding solution for eluting the DNA fragment of interest from the chromatin bound to streptavidin paramagnetic beads 114. Droplet 112e may be composed of a wash buffer solution for washing away unbound reagents with the minimal loss of any DNA fragments of interest from functionalized paramagnetic beads 124. It can be appreciated that the hydrophilic nature of the array of hydrophilic spots 110a-111e on ELR surface 28 act to pin droplets 112a-112e thereon. In addition, the hydrophobic nature of ELR surface 28 further acts to retain droplets 112a-112e on hydrophilic spots 110a-110e of ELR surface 28.

[0055] In operation, injector 34 delivers droplet 120 of a desired volume, e.g., 2 μ L, containing cells 122 and streptavidin paramagnetic beads 14 into reservoir 22. As heretofore described, magnetic manipulator 42 is configured to interact magnetically with streptavidin paramagnetic beads 114 within droplet 120 to initiate movement of the droplet 120. As such, magnetic manipulator 42 may be utilized to draw droplet 120 over first location 102 of the previously dried nuclear isolation buffer. With droplet 120 positioned over first location 102 of the previously dried nuclear isolation buffer, droplet 120 picks-up and re-dissolves the nuclear isolation buffer over a desired incubation period, with virtually no increase in the total volume of droplet 120. By exposing cells 122 to the nuclear isolation buffer, the nuclear fraction of cells 122 are isolated.

[0056] Once the nuclear fractions of cells 122 are isolated, magnetic manipulator 42 is utilized to draw droplet 120 over second location 104 of the previously dried MNase digestion solution. With droplet 120 positioned over second location 104 of the previously dried MNase digestion solution, droplet 120 picks-up and re-dissolves the MNase digestion solution over a desired incubation period, with virtually no increase in the total volume of droplet 120. The MNase digestion solution of droplet 120 fragments the chromatin complexes released from the nuclear fraction of cell lysates from cells 122.

[0057] After the chromatin are released from the nuclear fraction of cells 122 and chromatin 126 is sheared, magnetic manipulator 42 is utilized to draw droplet 120 over third location 106 of the previously dried EDTA/Triton/deoxy-

cholate solution. With droplet **120** positioned over third location **106** of the previously dried EDTA/Triton/deoxycholate solution, droplet **120** picks-up and re-dissolves the EDTA/Triton/deoxycholate solution over a desired incubation period, with virtually no increase in the total volume of droplet **120**. The EDTA/Triton/deoxycholate solution of droplet **120** facilitates the decellularization and solubilization of proteins contained in cells **122**.

[0058] Magnetic manipulator **42** then draws droplet **120** over hydrophilic spot **110a** such that droplet **120** communicates with and combines with droplet **112a**. With droplet **120** and droplet **112a** combined, biotinylated antibodies **128** bind to streptavidin paramagnetic beads **114** and to sheared chromatin **126**. With chromatin **126** bound to streptavidin paramagnetic beads **114** (through biotinylated antibodies **128**) in combined droplets **120** and **112a**, magnetic manipulator **42** is, once again, slid axially along the underside of ELR surface **28** to a position below hydrophilic spot **110b** such that the magnetic force generated by magnetic manipulator **42** draws streptavidin paramagnetic beads **114** from combined droplets **120** and **112a**, through oil **24**, and into droplet **112b**. Due to the immiscible characteristics of oil **24** and aqueous phase of combined droplets **120** and **112a**, the aqueous liquid is removed from streptavidin paramagnetic beads **114**, thereby greatly reducing the residual liquid adsorbed on streptavidin paramagnetic beads **114**. With streptavidin paramagnetic beads **114** received in droplet **112b**, low salt wash buffer solution of droplet **112b** washes away any undesired material from streptavidin paramagnetic beads **114** with the minimal loss of chromatin **126** bound to streptavidin paramagnetic beads **114**.

[0059] After the initial washing in droplet **112b**, magnetic manipulator **42** is slid axially along the underside of ELR surface **28** to a position below hydrophilic spot **110c** such that the magnetic force generated by magnetic manipulator **42** draws streptavidin paramagnetic beads **114** from droplet **112b**, through oil **24**, and into droplet **112c**. Due to the immiscible characteristics of oil **24** and aqueous phase of droplets **112b**, the aqueous liquid is removed from streptavidin paramagnetic beads **114**, thereby greatly reducing the residual liquid adsorbed on streptavidin paramagnetic beads **114**. With streptavidin paramagnetic beads **114** received in droplet **112c**, high salt wash buffer solution of droplet **112c** further washes away any undesired material from streptavidin paramagnetic beads **114** with the minimal loss of chromatin **126** bound to streptavidin paramagnetic beads **114**.

[0060] Once streptavidin paramagnetic beads **114** are washed in droplet **112c**, magnetic manipulator **42** is slid axially along the underside of ELR surface **28** to a position below hydrophilic spot **110d** of ELR surface **28**. The magnetic force generated by magnetic manipulator **42** draws streptavidin paramagnetic beads **114** from droplet **112c**, through oil **24**, and into droplet **112d**. Due to the immiscible characteristics of oil **24** and aqueous phase of droplet **112c**, the aqueous liquid is removed from streptavidin paramagnetic beads **114**, thereby greatly reducing the residual liquid adsorbed on streptavidin paramagnetic beads **114**. Elution buffer of droplet **112d** facilitates the elution of DNA **131** from chromatin **126** bound to streptavidin paramagnetic beads **114**. Streptavidin paramagnetic beads **114** may be removed from droplet **112d** by a magnetic force generated by a secondary magnetic force generator, e.g., magnet **130**. Thereafter, functionalized paramagnetic beads **124** are intro-

duced in droplet **112d**. Functionalized paramagnetic beads **124** are coated with a material, e.g. silica, such that DNA **131** binds thereto.

[0061] Once DNA **131** binds to functionalized paramagnetic beads **124**, magnetic manipulator **42** is slid axially along the underside of ELR surface **28** to a position below hydrophilic spot **110e** such that the magnetic force generated by magnetic manipulator **42** draws functionalized paramagnetic beads **124** from droplet **112d**, through oil **24**, and into droplet **112e**. Due to the immiscible characteristics of oil **24** and aqueous phase of droplet **112d**, the aqueous liquid is removed from functionalized paramagnetic beads **124**, thereby greatly reducing the residual liquid adsorbed on functionalized paramagnetic beads **124**. With functionalized paramagnetic beads **124** received in droplet **112e**, wash buffer solution of droplet **112e** washes away any undesired material from functionalized paramagnetic beads **124** with the minimal loss of DNA **131** bound thereto.

[0062] After functionalized paramagnetic beads **124** are washed, injector **34** delivers droplet **132** of an elution buffer having a desired volume into reservoir **22**. Magnetic manipulator **42** is slid axially along the underside of ELR surface **28** so as to draw functionalized paramagnetic beads **124** from droplet **112**, through oil **24**, and into droplet **132**. Due to the immiscible characteristics of oil **24** and aqueous phase of droplet **112e**, the aqueous liquid is removed from functionalized paramagnetic beads **124**, thereby greatly reducing the residual liquid adsorbed on functionalized paramagnetic beads **124**. Elution buffer of droplet **132** facilitates the elution of DNA **131** from functionalized paramagnetic beads **124**. Once DNA **131** is eluted from functionalized paramagnetic beads **124**, DNA **131** may be removed from droplet **132** for further downstream processing.

[0063] Various modes of carrying out the invention are contemplated as being within the scope of the following claims particularly pointing out and distinctly claiming the subject matter that is regarded as the invention.

We claim:

1. A method of sample preparation for streamlined multi-step assays, comprising the steps:
 - providing a microfluidic device including a reservoir defined by a surface configured to repel an aqueous solution;
 - providing a dried reagent on a portion of the surface;
 - filling the reservoir with an oil; and
 - positioning a droplet of the aqueous solution on the dried reagent, the droplet picking-up and re-dissolving the dried reagent therein so as to expose the portion of the surface.
2. The method of claim **1** wherein the step of providing the dried reagent on the portion of the surface comprises the additional steps:
 - depositing the reagent on the surface; and
 - allowing reagent to dry and physically adsorb onto surface.
3. The method of claim **1** wherein the droplet includes paramagnetic beads therein.
4. The method of claim **3** wherein the step of positioning the droplet of the aqueous solution on the dried reagent includes the steps of:
 - generating a magnetic force; and
 - positioning the magnetic force interact magnetically with the paramagnetic beads within the droplet; and

- moving the magnetic force to initiate corresponding movement of the droplet to the portion of the surface.
5. The method of claim 4 comprising the additional step of patterning a hydrophilic spot on the surface at a second location.
6. The method of claim 5 wherein the portion of the surface is a hydrophilic spot.
7. The method of claim 5 comprising the additional step of moving the droplet with the dissolved reagent to the hydrophilic spot.
8. The method of claim 7 wherein the droplet is pinned at the hydrophilic spot.
9. The method of claim 7 wherein the step of moving the droplet with the dissolved reagent to the hydrophilic spot includes the additional steps of:
- positioning the magnetic force to interact magnetically with the paramagnetic beads within the droplet; and
 - moving the magnetic force to initiate corresponding movement of the droplet to the hydrophilic spot.
10. The method of claim 9 wherein the hydrophilic spot is a first hydrophilic spot and wherein the method comprises the additional step of patterning a second hydrophilic spot on the surface at a third location.
11. The method of claim 10 wherein the aqueous solution is a first aqueous solution and the droplet is a first droplet and wherein the method further comprises the additional step of pinning a second droplet of the second solution at the second hydrophilic spot.
12. The method of claim 11 further comprising the additional steps of:
- positioning the magnetic force to interact magnetically with the paramagnetic beads within the first droplet; and
 - moving the magnetic force to initiate corresponding movement of the paramagnetic beads from the first droplet to the second droplet.
13. The method of claim 4 wherein the dried reagent is a first dried reagent and the portion of the surface is a first portion and wherein the method further comprises the additional step of providing a second dried reagent on a second portion of the surface.
14. The method of claim 12 wherein the step of providing the second dried reagent on the second portion of the surface comprises the additional steps:
- depositing the second reagent on the second portion of the surface; and
 - allowing second reagent to dry and physically adsorb onto the second portion of the surface.
15. The method of claim 13 comprising the additional steps of:
- positioning the magnetic force interact magnetically with the paramagnetic beads within the droplet; and
 - moving the magnetic force to initiate corresponding movement of the droplet to the second portion of the surface.
16. The method of claim 14 comprising the additional step of picking-up and re-dissolving the second dried reagent in the droplet so as to expose the second portion of the surface.
17. A method of sample preparation for streamlined multi-step assays, comprising the steps:
- providing a microfluidic device including a reservoir defined by a surface configured to repel aqueous solutions;
 - patterning first and second hydrophilic spots at corresponding first and second locations of the surface;
 - filling the reservoir with an oil;
 - depositing a first droplet of a first aqueous solution on the first hydrophilic spot and a second droplet of a second aqueous solution on the second hydrophilic spot, the first droplet including paramagnetic beads;
 - generating a magnetic force configured to interact magnetically with the paramagnetic beads within the first droplet; and
 - moving the magnetic force to initiate corresponding movement of the paramagnetic beads from the first droplet, through the oil, into the second droplet.
18. The method of claim 17 further comprising the step of providing a dried reagent at a third location the surface prior to filling the reservoir with oil.
19. The method of claim 18 wherein the step of providing the dried reagent on the portion of the surface comprises the additional steps:
- depositing the reagent in a third aqueous solution on the surface; and
 - allowing the third aqueous solution to dry such that a dried reagent is physically adsorbed onto surface.
20. The method of claim 19 comprising the additional step of positioning a third droplet of a third aqueous solution on the dried reagent, the third droplet picking-up and re-dissolving the dried reagent therein so as to expose the portion of the surface.
21. The method of claim 20 wherein the paramagnetic beads are initially in the third droplet and wherein the method comprises the additional steps of:
- positioning the magnetic force to interact magnetically with the paramagnetic beads within the third droplet; and
 - moving the magnetic force to initiate corresponding movement of the paramagnetic beads from the third droplet, through the oil, into the first droplet.
22. The method of claim 20 wherein the paramagnetic beads are initially in the third droplet and wherein the method comprises the additional steps of:
- positioning the magnetic force to interact magnetically with the paramagnetic beads within the third droplet; and
 - moving the magnetic force to initiate corresponding movement of the third droplet into fluid communication with the first droplet.
23. The method of claim 20 comprising the additional steps of:
- positioning the magnetic force to interact magnetically with the paramagnetic beads within the second droplet; and
 - moving the magnetic force to initiate corresponding movement of the paramagnetic beads from the second droplet, through the oil, into the third droplet.
24. The method of claim 23 comprising the additional step of
- positioning the magnetic force to interact magnetically with the paramagnetic beads within the third droplet; and
 - causing the magnetic force to initiate movement of the paramagnetic beads from the third droplet.
25. The method of claim 17 wherein the first droplet is pinned at the first hydrophilic spot and the second droplet is pinned at the second hydrophilic spot.

26. The method of claim 17 comprising the additional steps of drying a first reagent on the first hydrophilic spot and drying the second reagent on the second hydrophilic spot.

* * * * *